


24844






PCB Piezotronics Inc. claims proprietary rights in the information disclosed hereon. Neither it nor any reproduction thereof will be disclosed to others without the written consent of PCB Piezotronics Inc.

REVISIONS		
REV	DESCRIPTION	DIN
B	UPDATED TITLE BLOCK	50900

INSTALLED WITHOUT "O-RING"

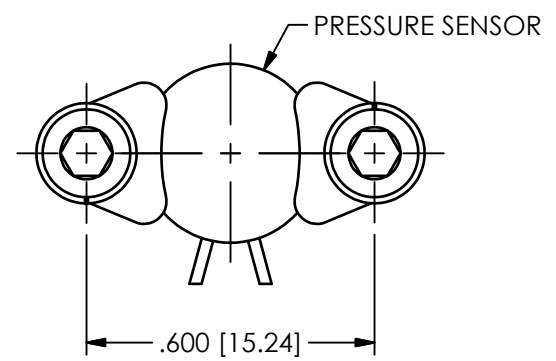

INSTALLED WITH ADHESIVE MOUNTING RING

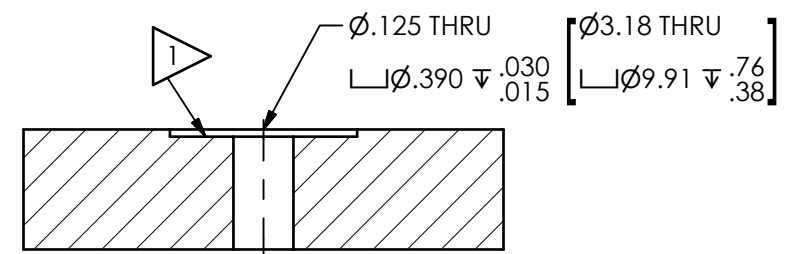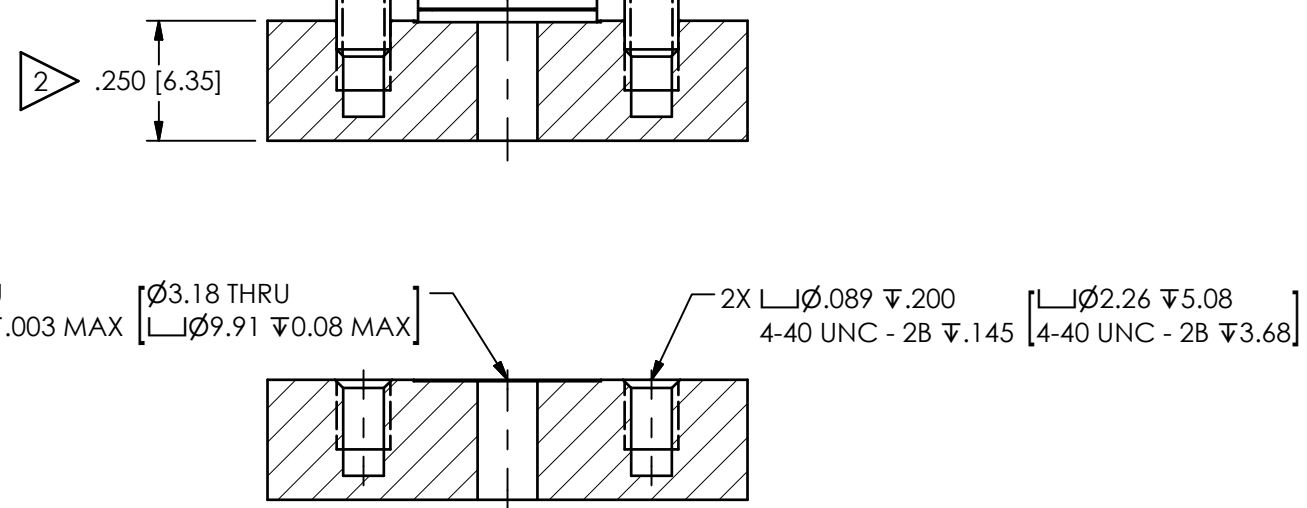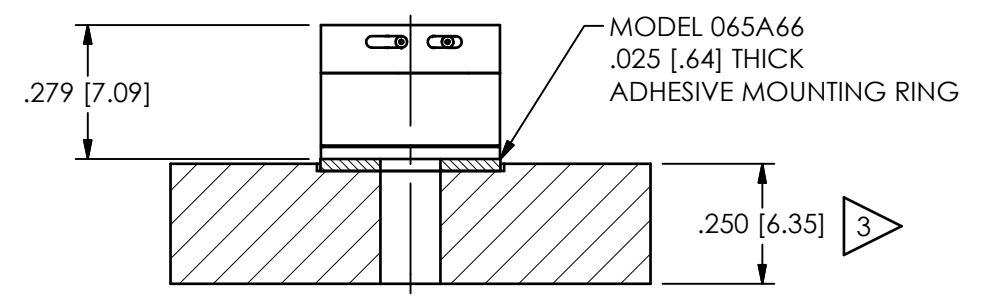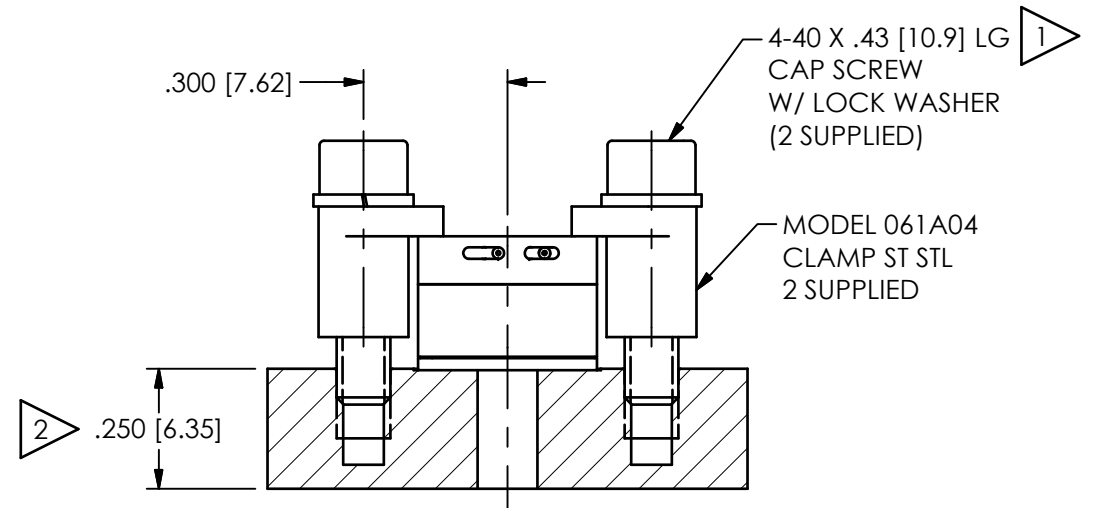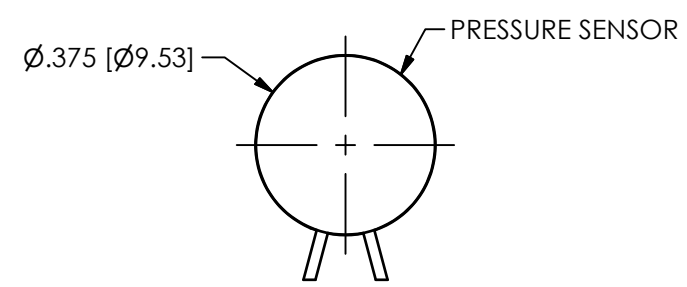

3) PREP SURFACE WITH A Ø.500[12.70] SPOTFACE, .015-.030 [.38-.76] x, 32 FINISH MIN. CENTER SPOTFACE TO .125[3.18]. APPLY 065A66 ADHESIVE MOUNTING RING, THEN SENSOR. LET SELF-CURE FOR 12 HRS. PRIOR TO TESTING. MAKE SURE SURFACE IS FREE OF DIRT, OIL, AND DEBRIS BEFORE APPLICATION.

2.) PRESSURE SHOULD NOT EXCEED 20 PSI WHEN USING ADHESIVE MOUNTING RING

1) EXCEEDING THIS DIMENSION WILL START LOWERING FREQUENCY RESPONSE

2) EXCEEDING THIS DIMENSION WILL START LOWERING FREQUENCY RESPONSE  
 1) MOUNTING TORQUE SHOULD BE BETWEEN 4-5 in-lbs [4.5-5.6 Nm]

UNLESS OTHERWISE SPECIFIED TOLERANCES ARE:		DRAWN		CHECKED		ENGINEER	
DIMENSIONS IN INCHES	DIMENSIONS IN MILLIMETERS [IN BRACKETS]	JDM	7/8/20	JDM	7/8/20	RF	7/8/20
DECIMALS XX ±.01 XXX ±.005	DECIMALS X ±.03 XX ±.013	TITLE INSTALLATION DRAWING PRESSURE SENSOR					
ANGLES ± 2 DEGREES	ANGLES ± 2 DEGREES						
FILLETS AND RADII .003 - .005	FILLETS AND RADII 0.07 - 0.13	CODE IDENT. NO. 52681		DWG. NO. 24844		SCALE: 2.5X SHEET 1 OF 1	

**PCB PIEZOTRONICS™**  
 3425 WALDEN AVE. DEPEW, NY 14043  
 (716) 684-0001 E-MAIL: sales@pcb.com